


## Modifying Monitored Values

Physiological parameters documented on the Anaesthesia Record can be modified in events where they are widely out of range caused by for example; SpO<sub>2</sub> probe falling off or high HR artifact during diathermy.

1. Right click on dot in graph to be changed.

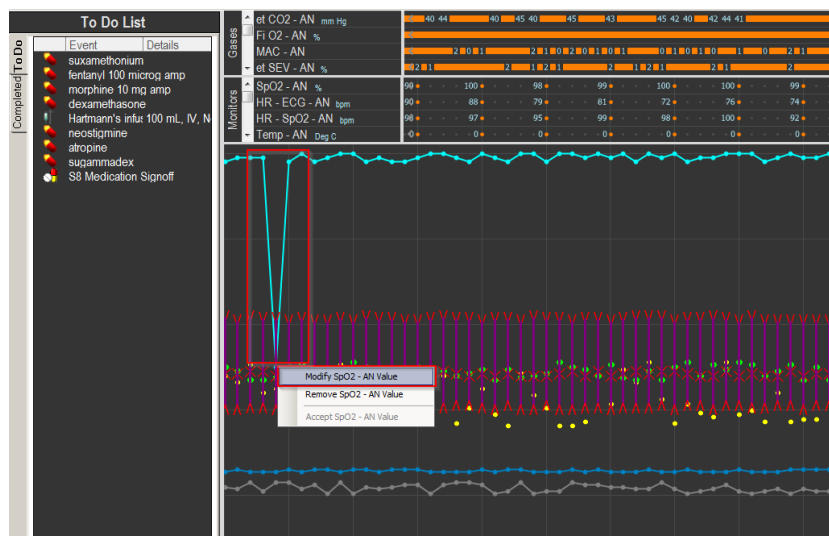

2. Click **Modify SpO2- AN Value.**
3. The Modify Monitor Value window pops up.

4. Type in correct value OR use the keypad displayed.
5. Click **OK.**

6. The value will be modified and seen on the graph.

